

Chemical Information:

Name: Anthralin
CAS No.: 1143-38-0
Tox21_ID No.: Tox21_201851
NTP_CID No.: 497

Supplier: Sigma-Aldrich
Lot No.: 054K3697
MW: 226.23 g/mol

Date of Analysis: 05 October 2007

Purity and Identity Results:


Peak Identity	Retention Time (min)	Purity (% Total Area) ^a
DMSO	5.17	Not applicable
Anthralin	21.79	98.64
unknown	25.62	0.90

^a Peaks comprising $\geq 0.5\%$ of total area.

GC/MS Instrument Parameters:


Instrument / Ionization	Gas Chromatograph / Mass Spectrometer / Electron Impact
Solvent	Dichloromethane (100 mM in DMSO, diluted 1/1000 with dichloromethane)
Column	J&W Scientific HP-5MS, 30 m x 0.25 mm ID, 0.25- μ m film thickness
Carrier Gas	Helium at 1.0 mL/min
Oven Program	35°C, hold 2 min; ramp @ 10°C/min to 310°C, hold 2 min
Source Temperature	250°C
Auxiliary Temperature	250°C
Scan Range	50 – 350 amu
Injector Temperature	250°C
Injection Volume / Mode	2 μ L / Splitless
Run Time	31.5 minutes
Data Analysis Software	Xcalibur, v 1.2 and NIST Library v 1.7, build 11/5/1999

RT: 3.05 - 31.50 SM: 3G

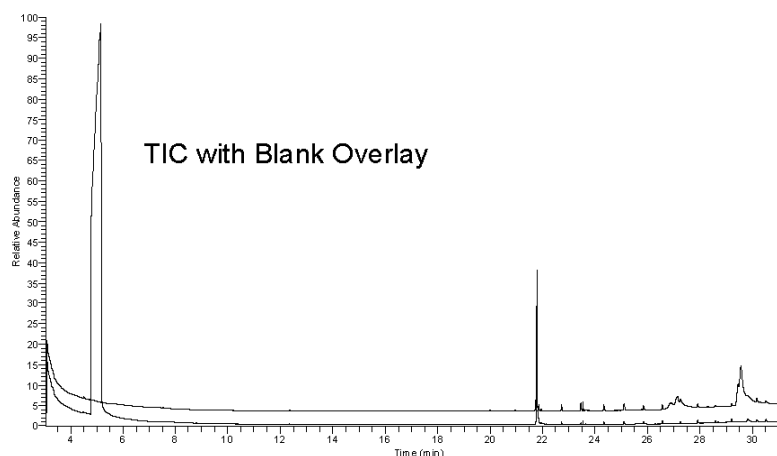

070597 #2253 RT: 21.79 MS: 1.73E6
T: (p) - c:11 det:350.00 Full.ms [58000.000]

Major Component Mass Spectrum

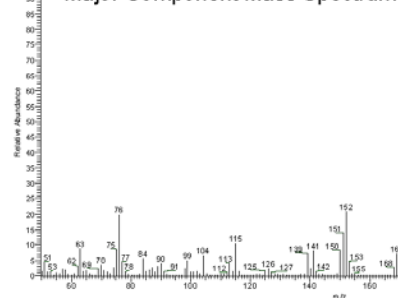

NIST Reference Mass Spectrum

